



300

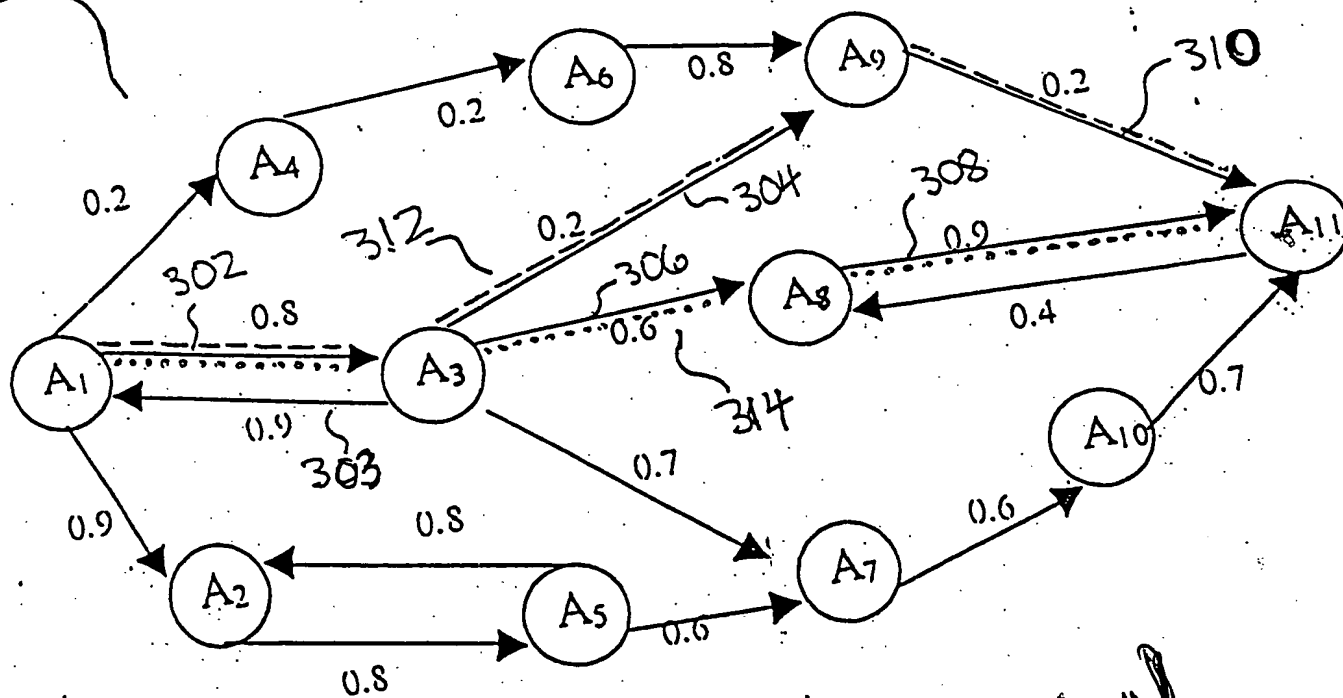


Fig. 1 (Prior Art)

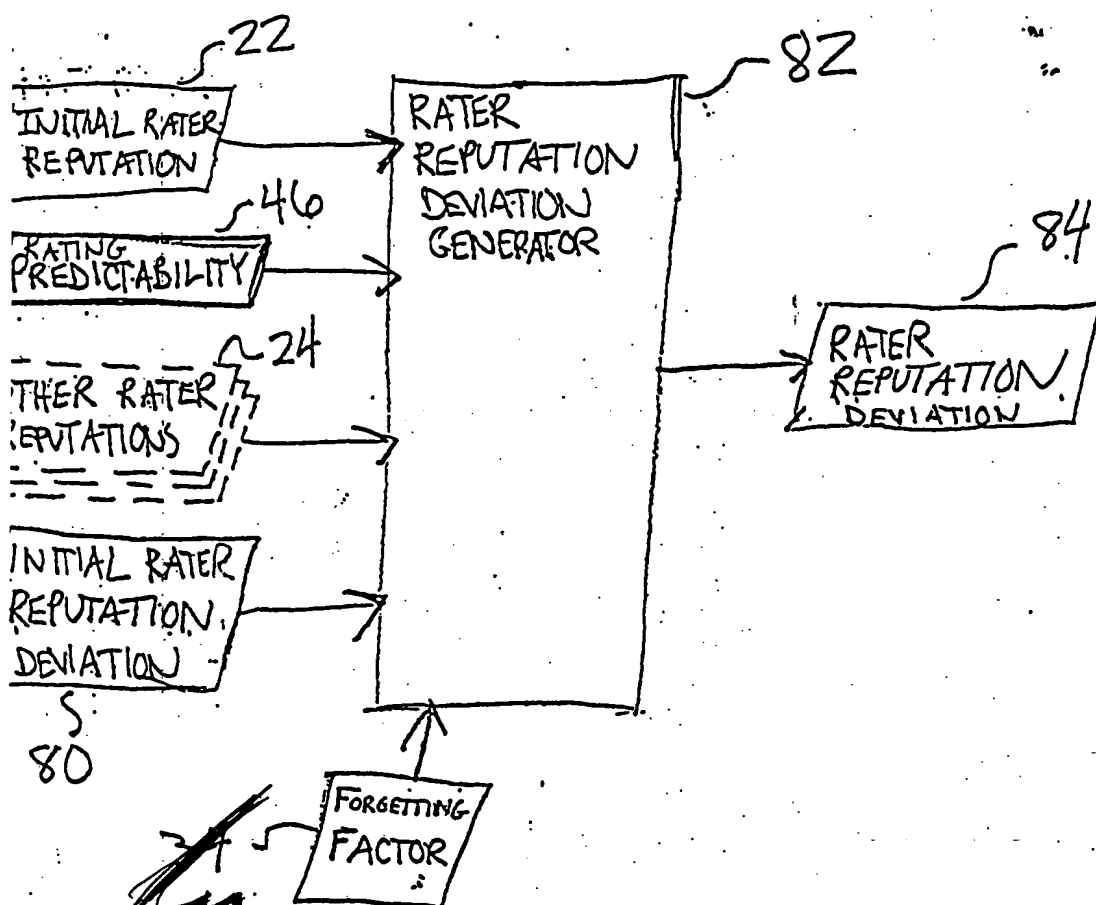


FIG. 7

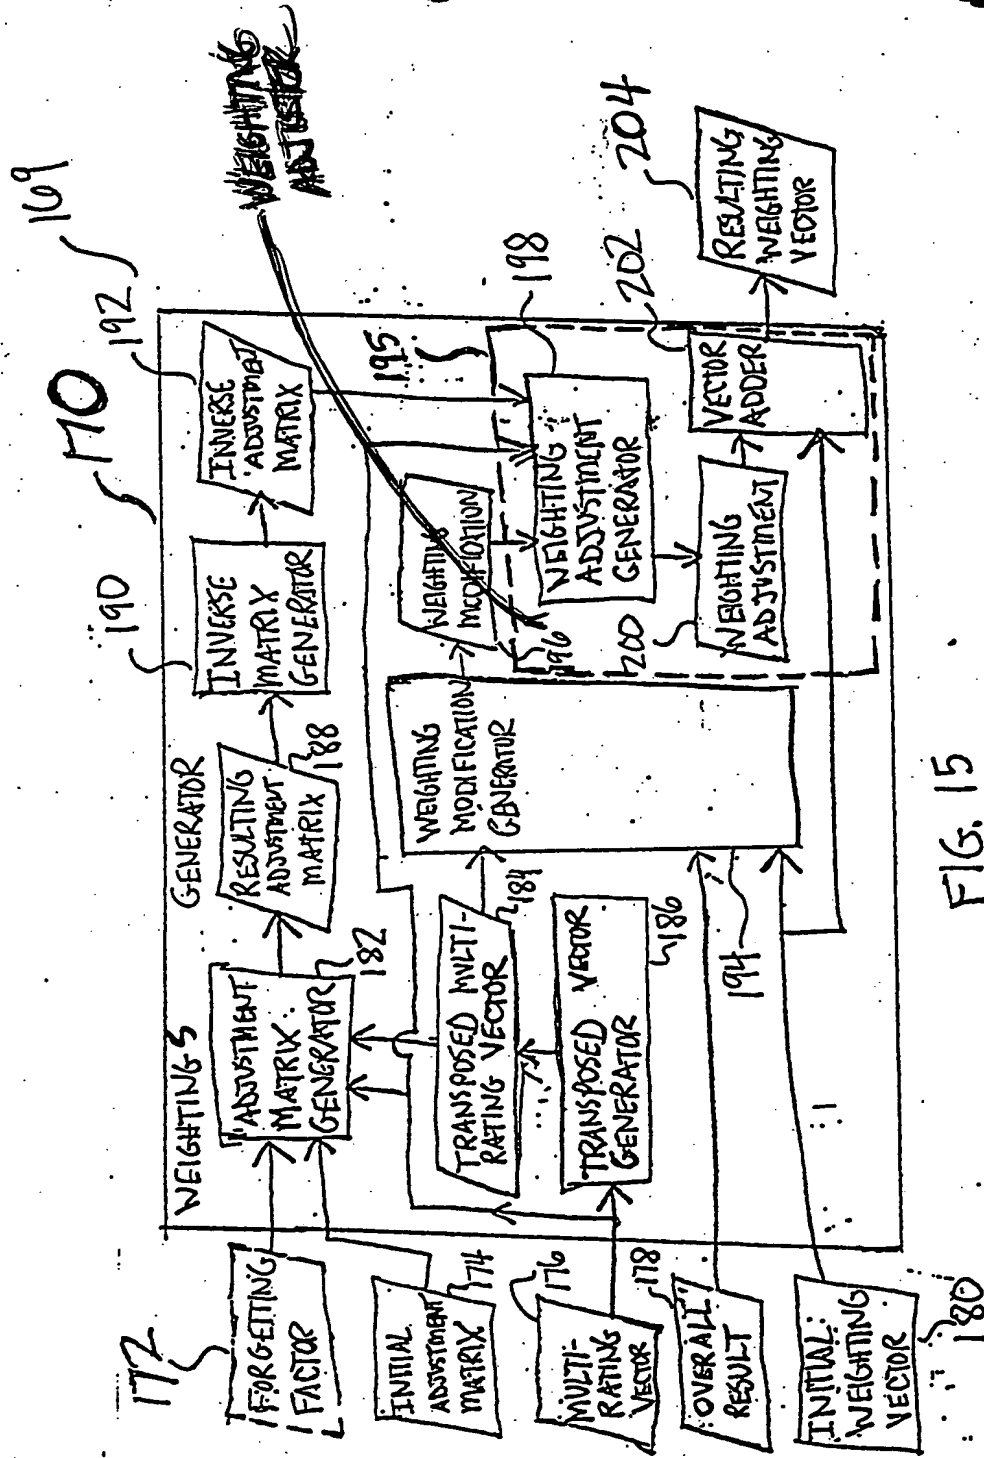


FIG. 15


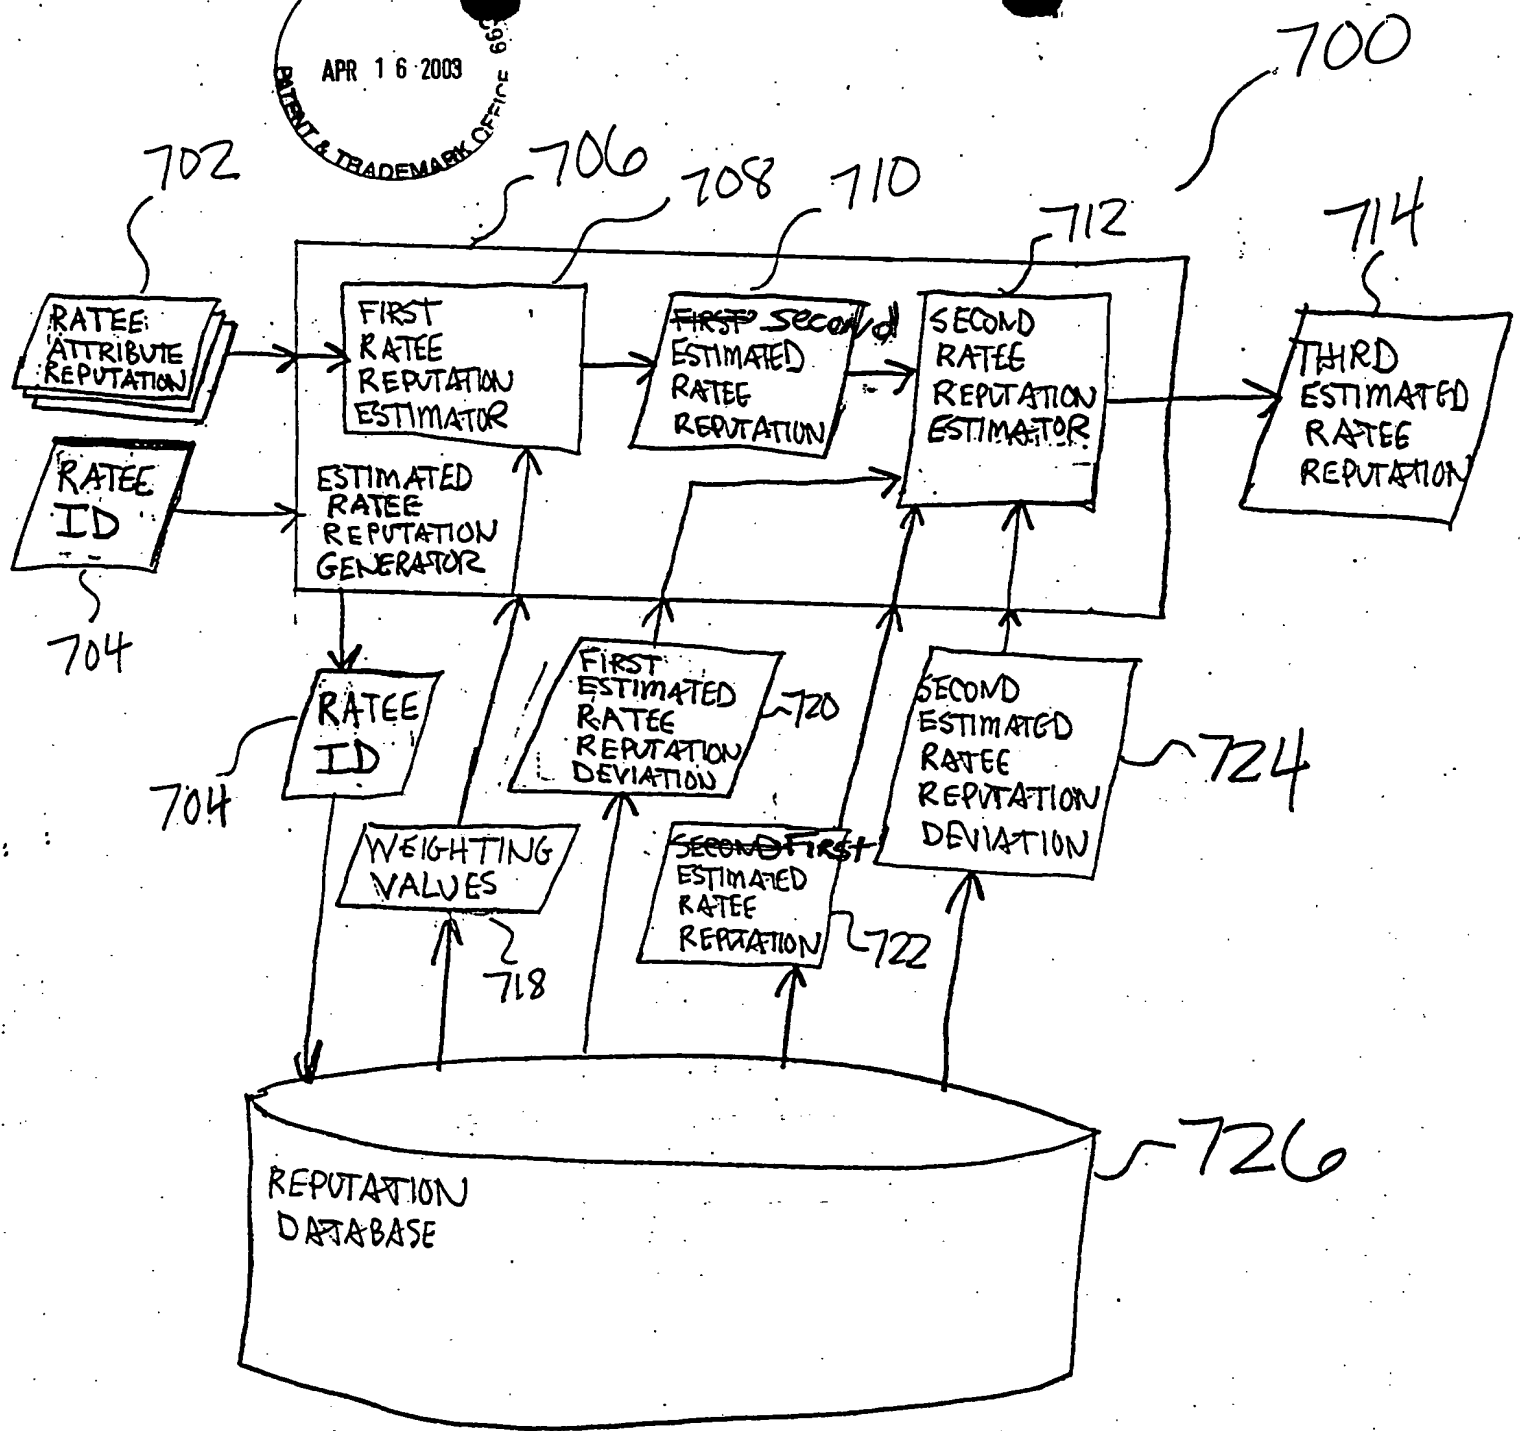


Fig. 17



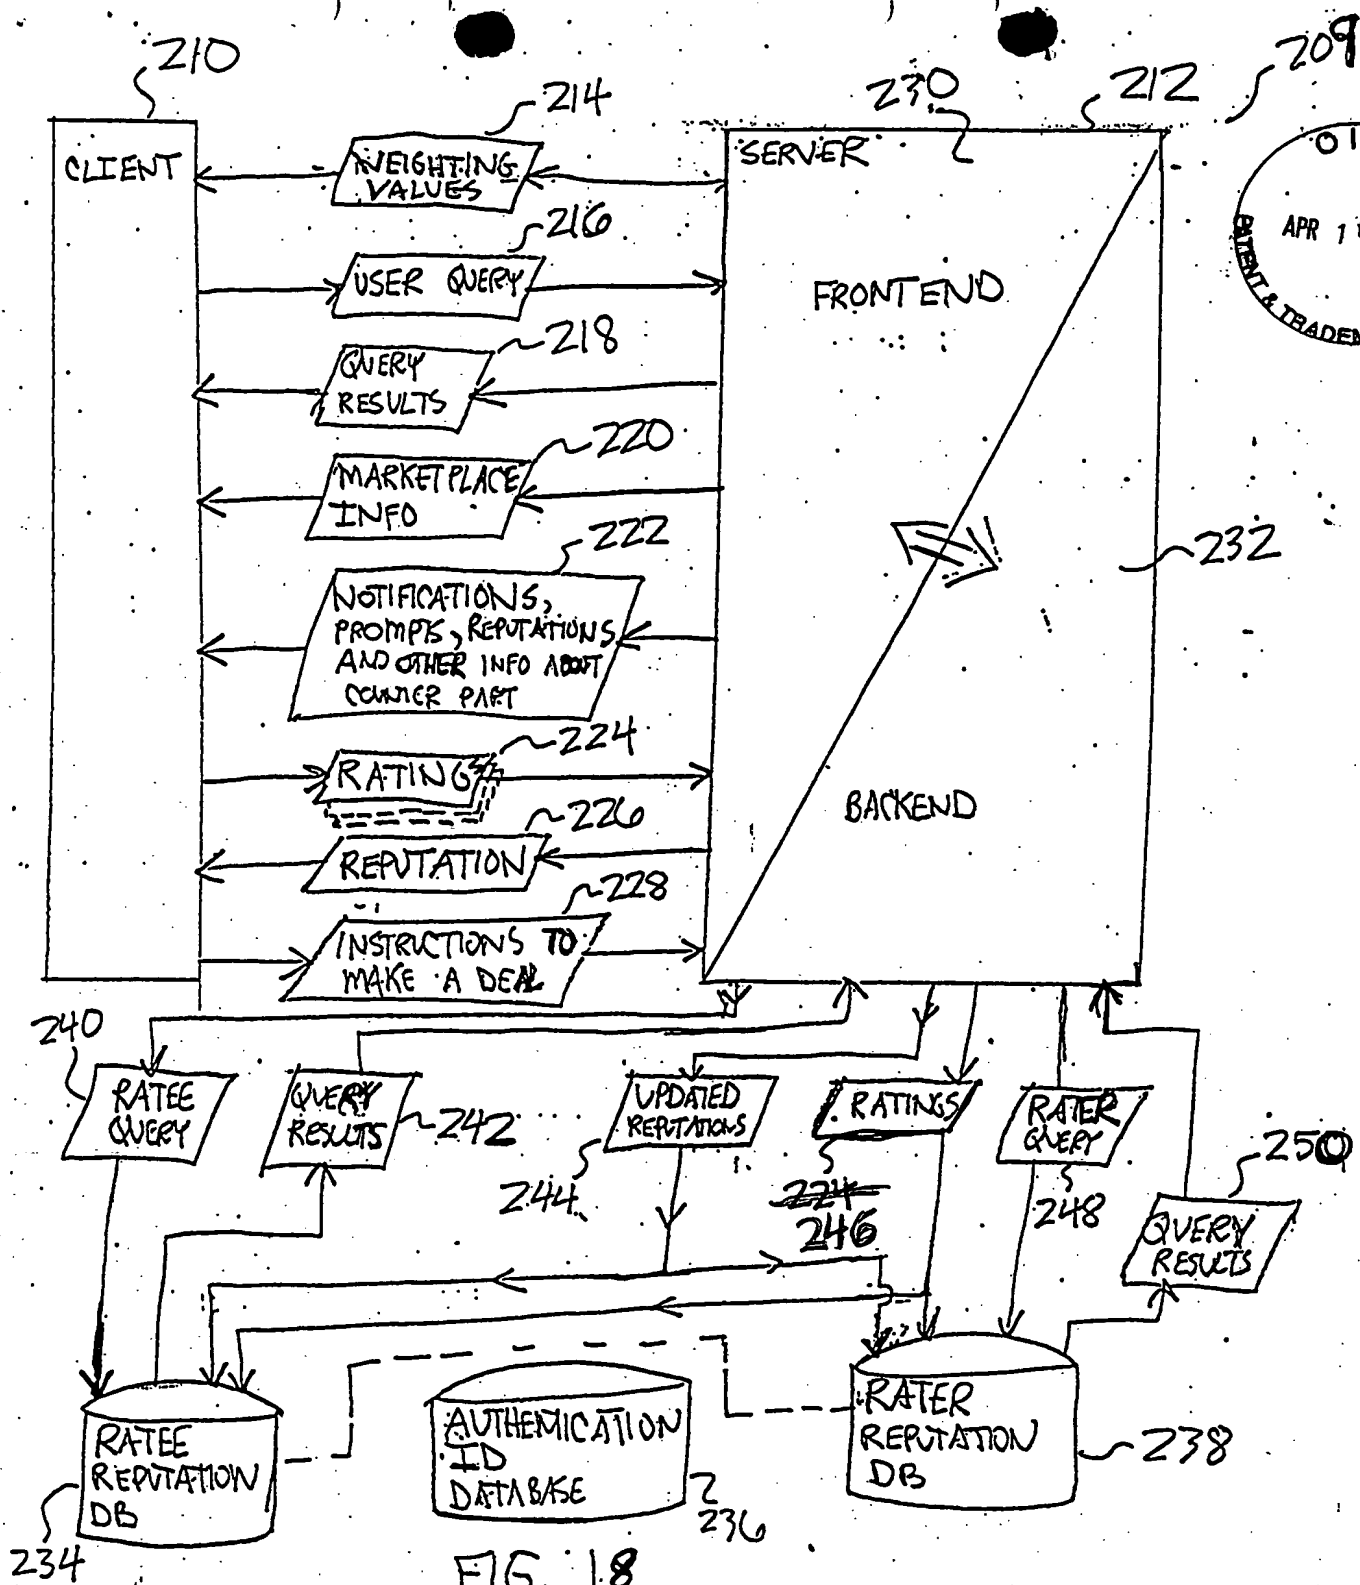

1/19


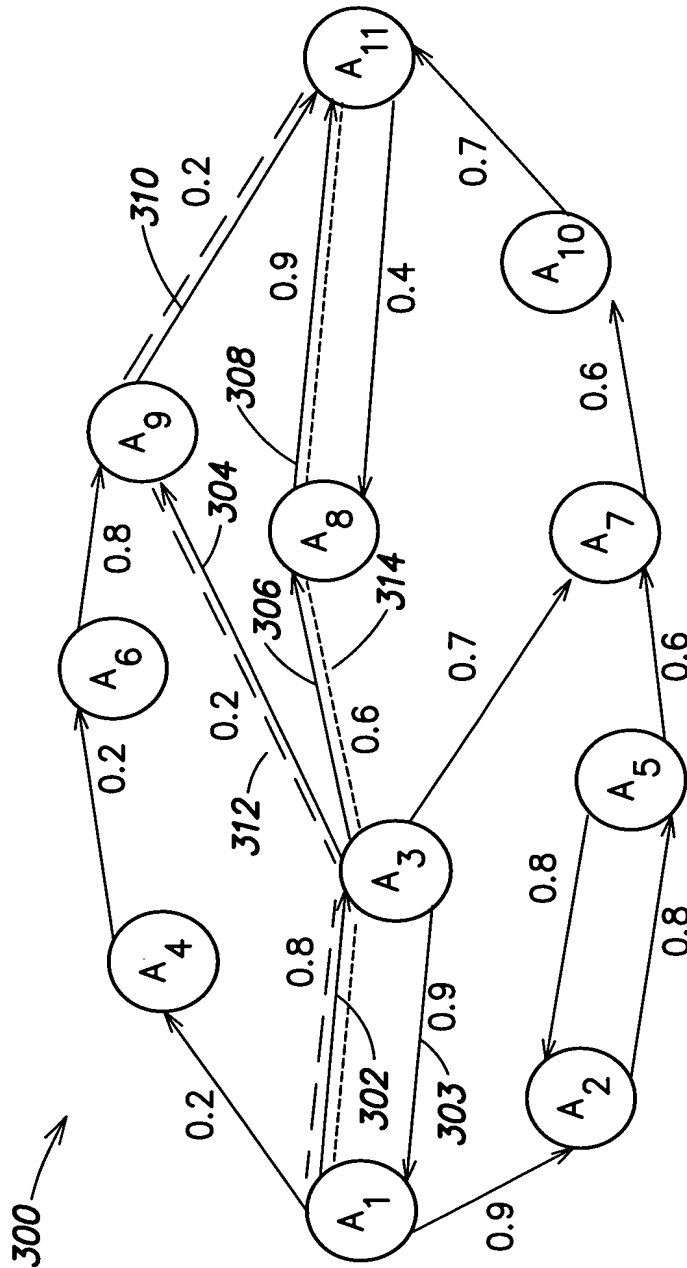


FIG. 1  
(PRIOR ART)




2/19

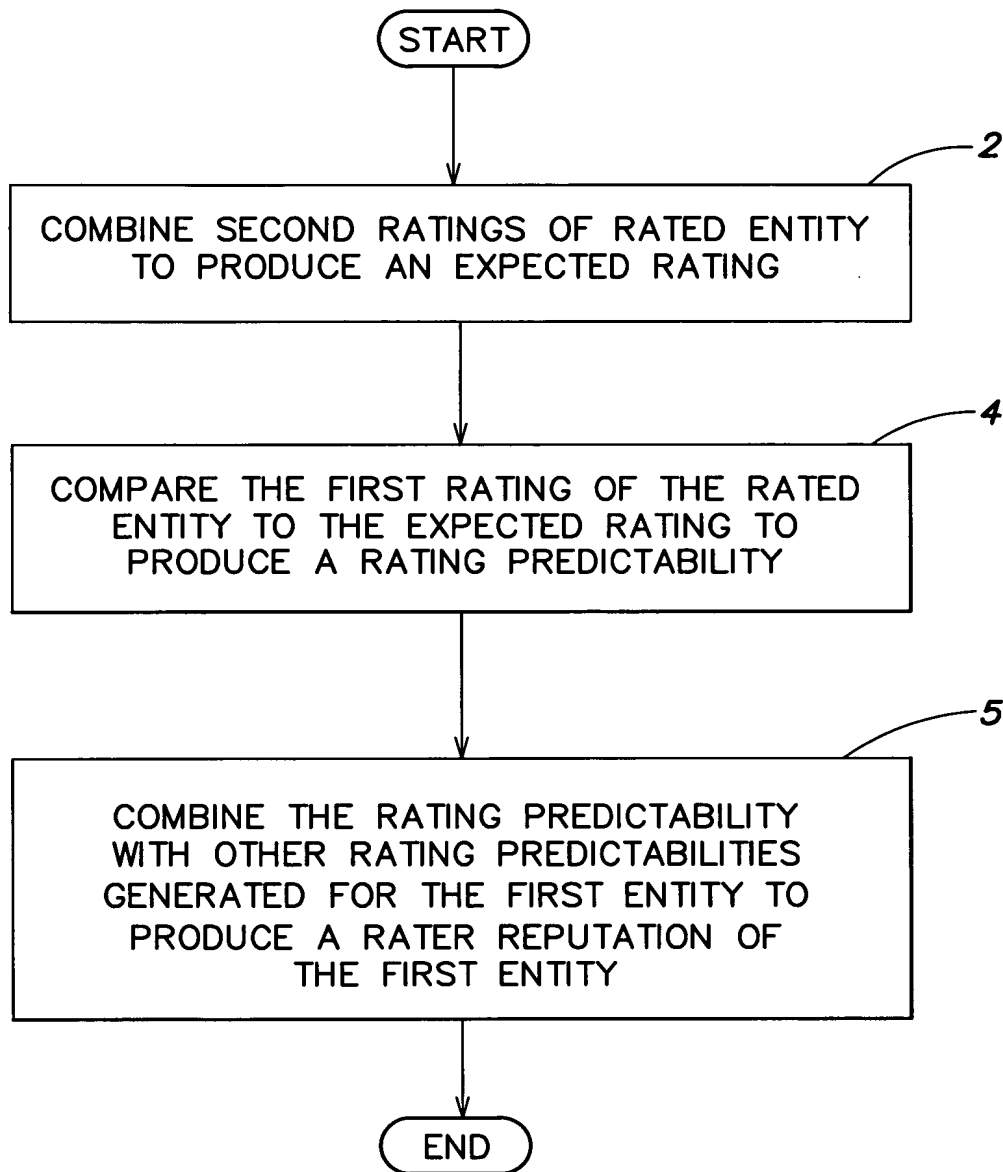

**FIG. 2**



3/19

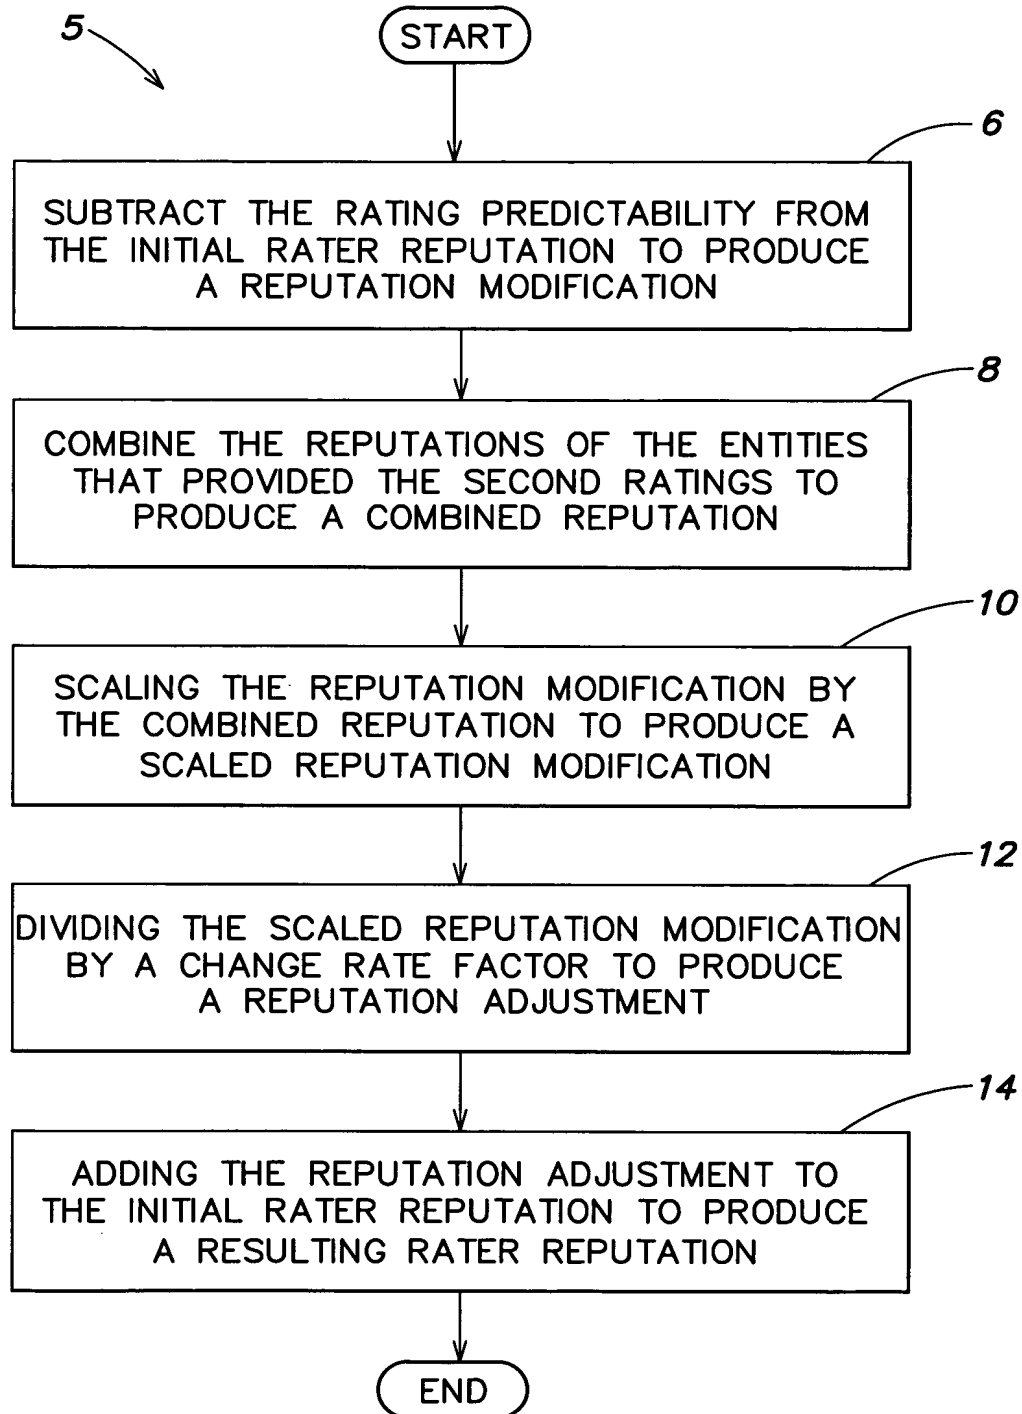

**FIG. 3**

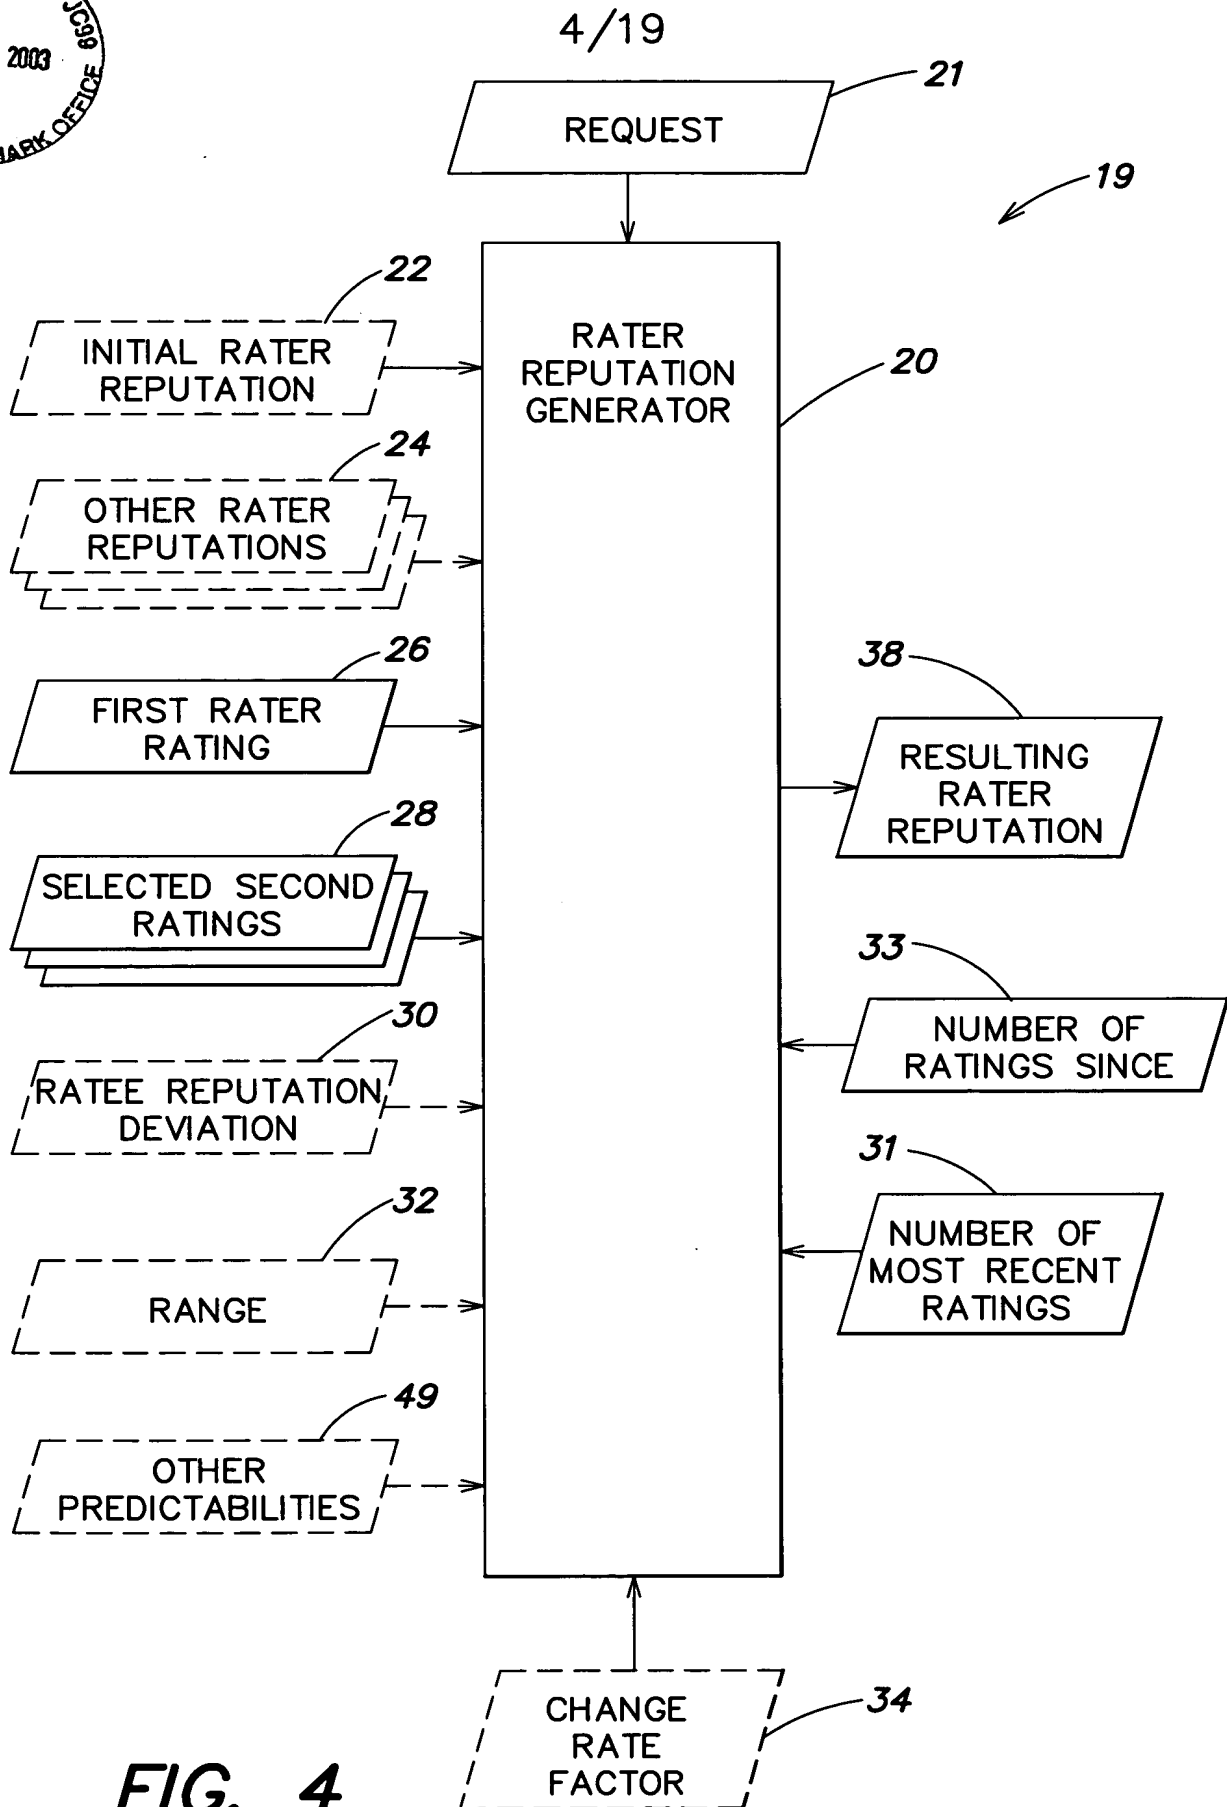


FIG. 4





6/19


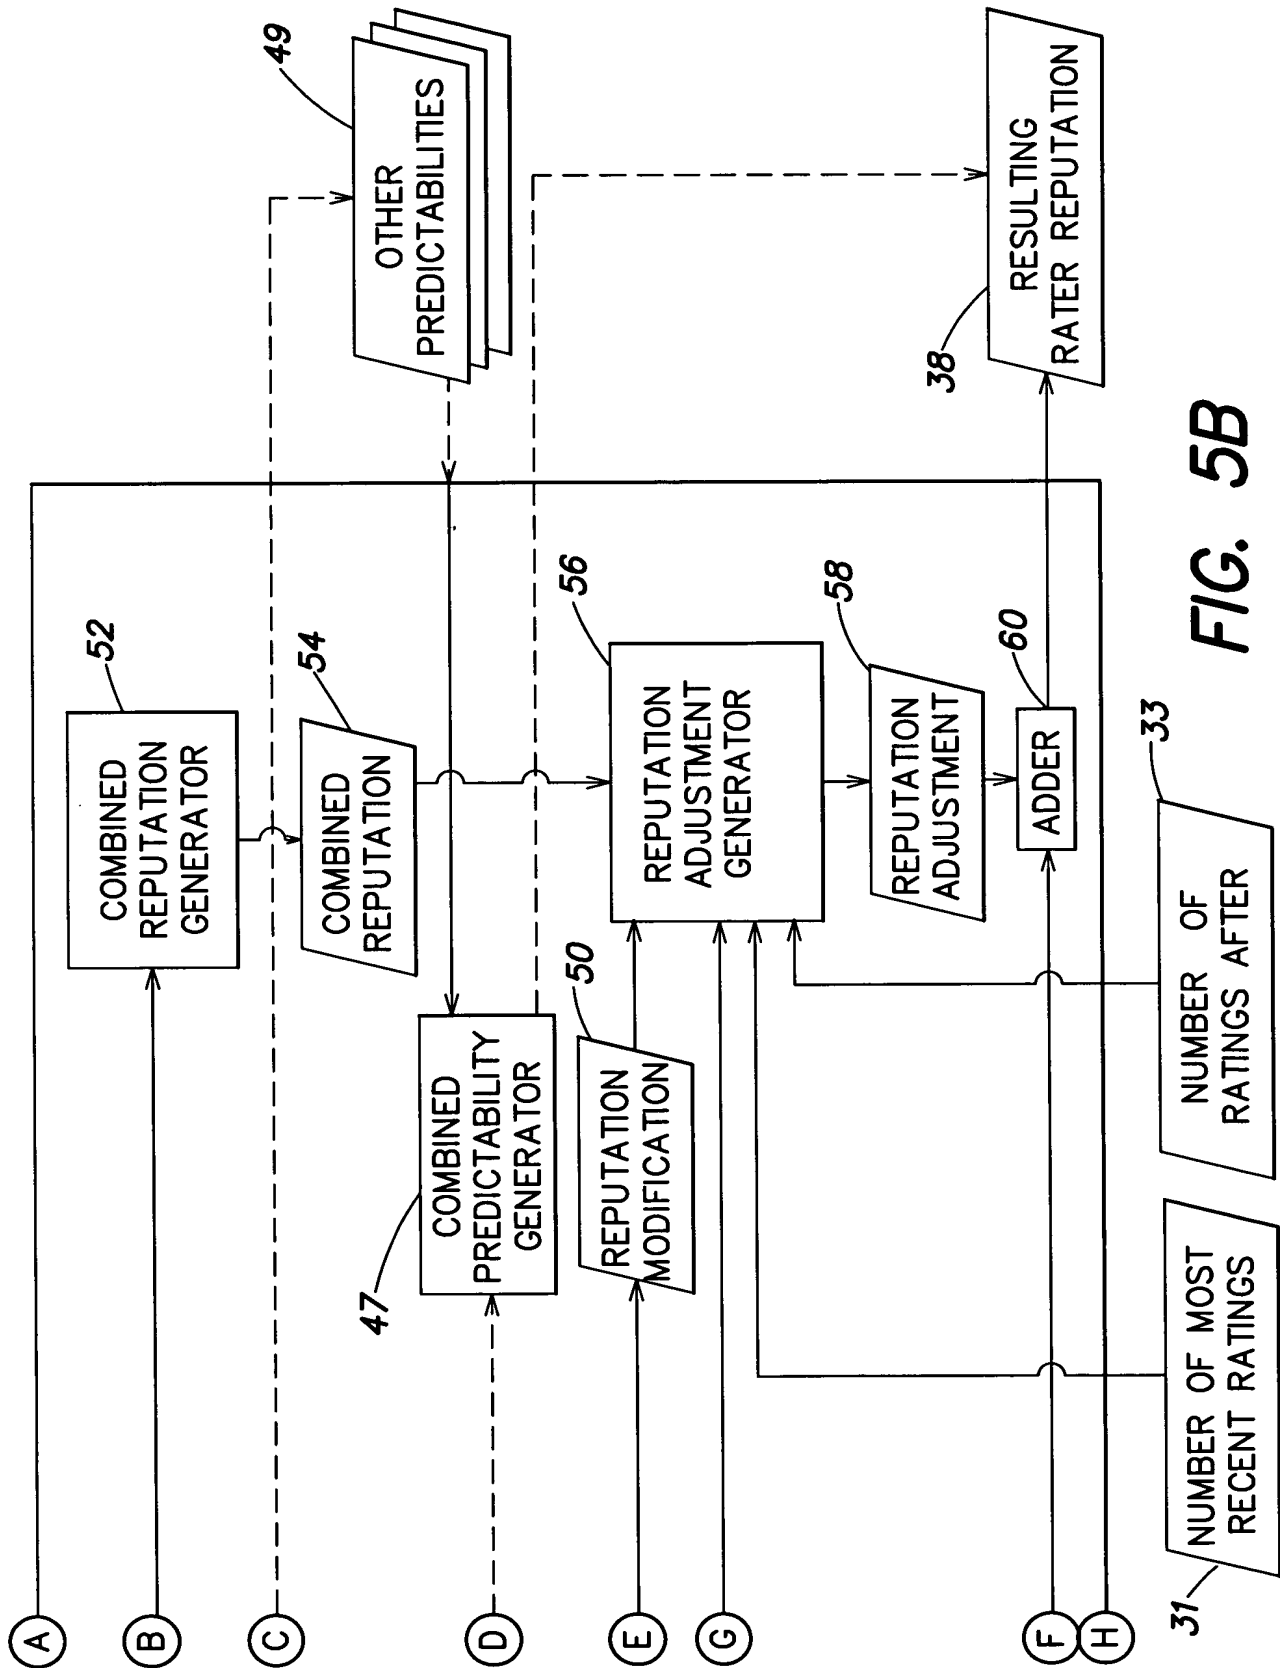


FIG. 5B



7/19


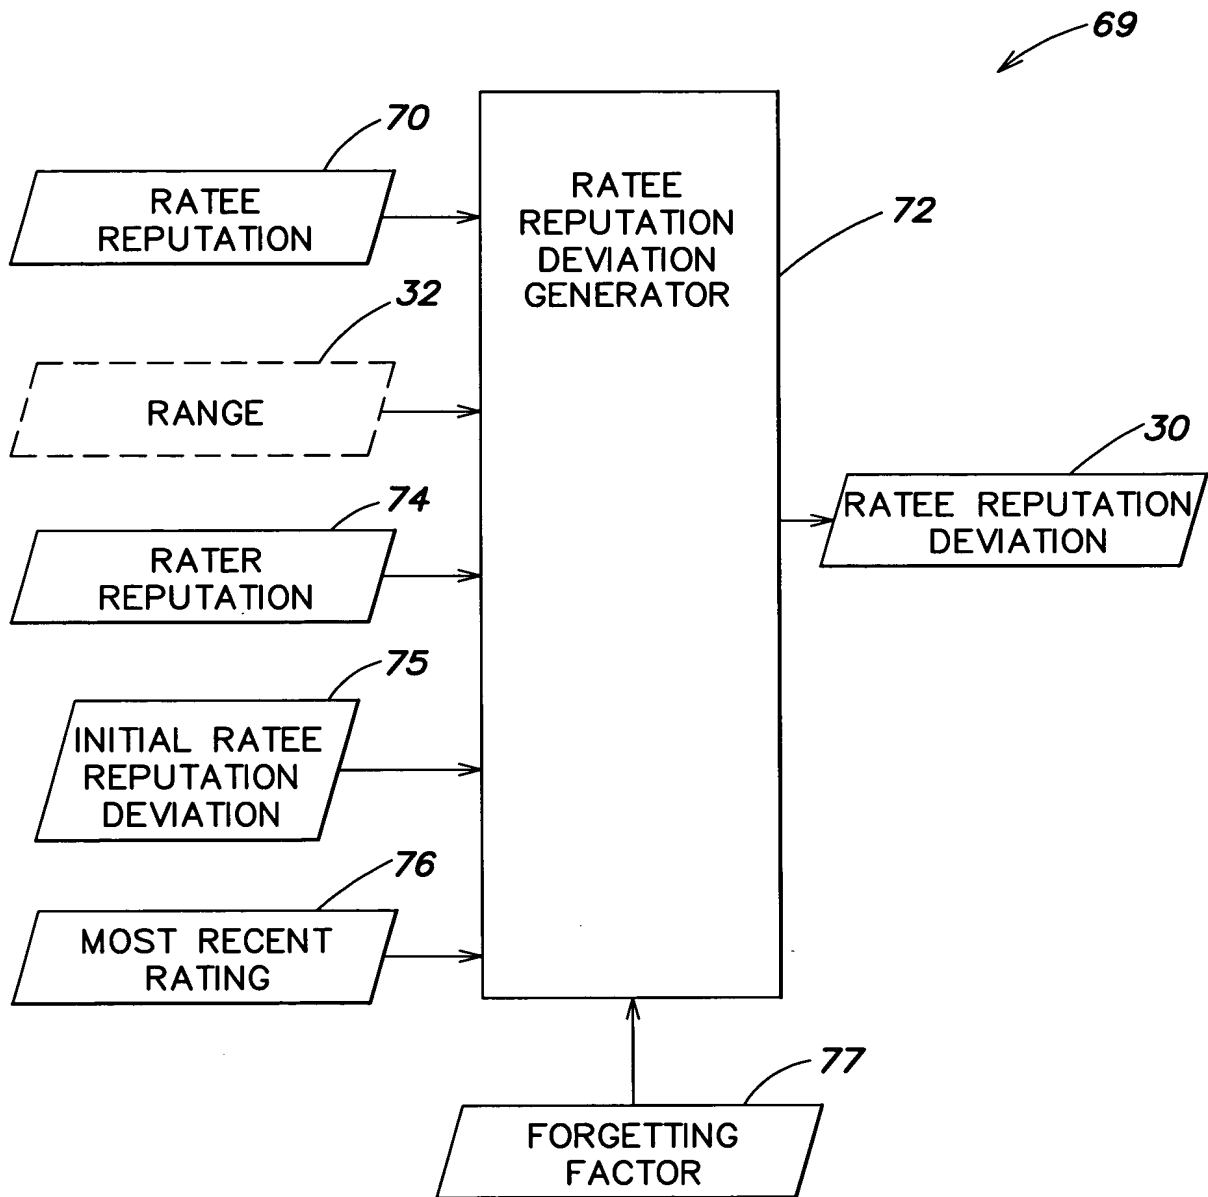


FIG. 6




8/19

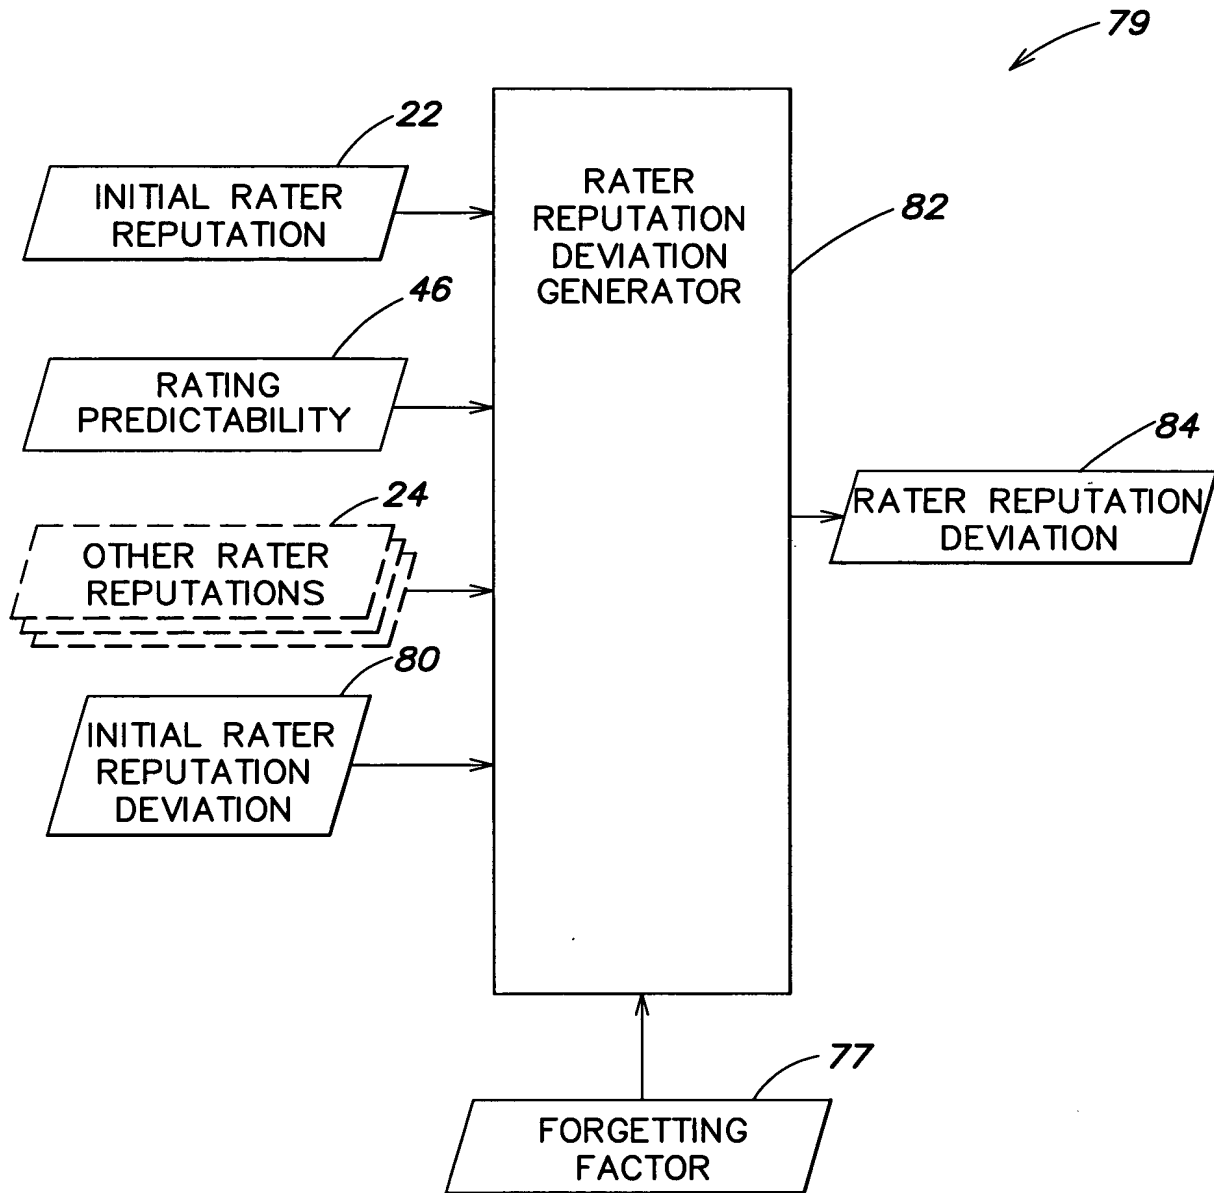

**FIG. 7**



9/19

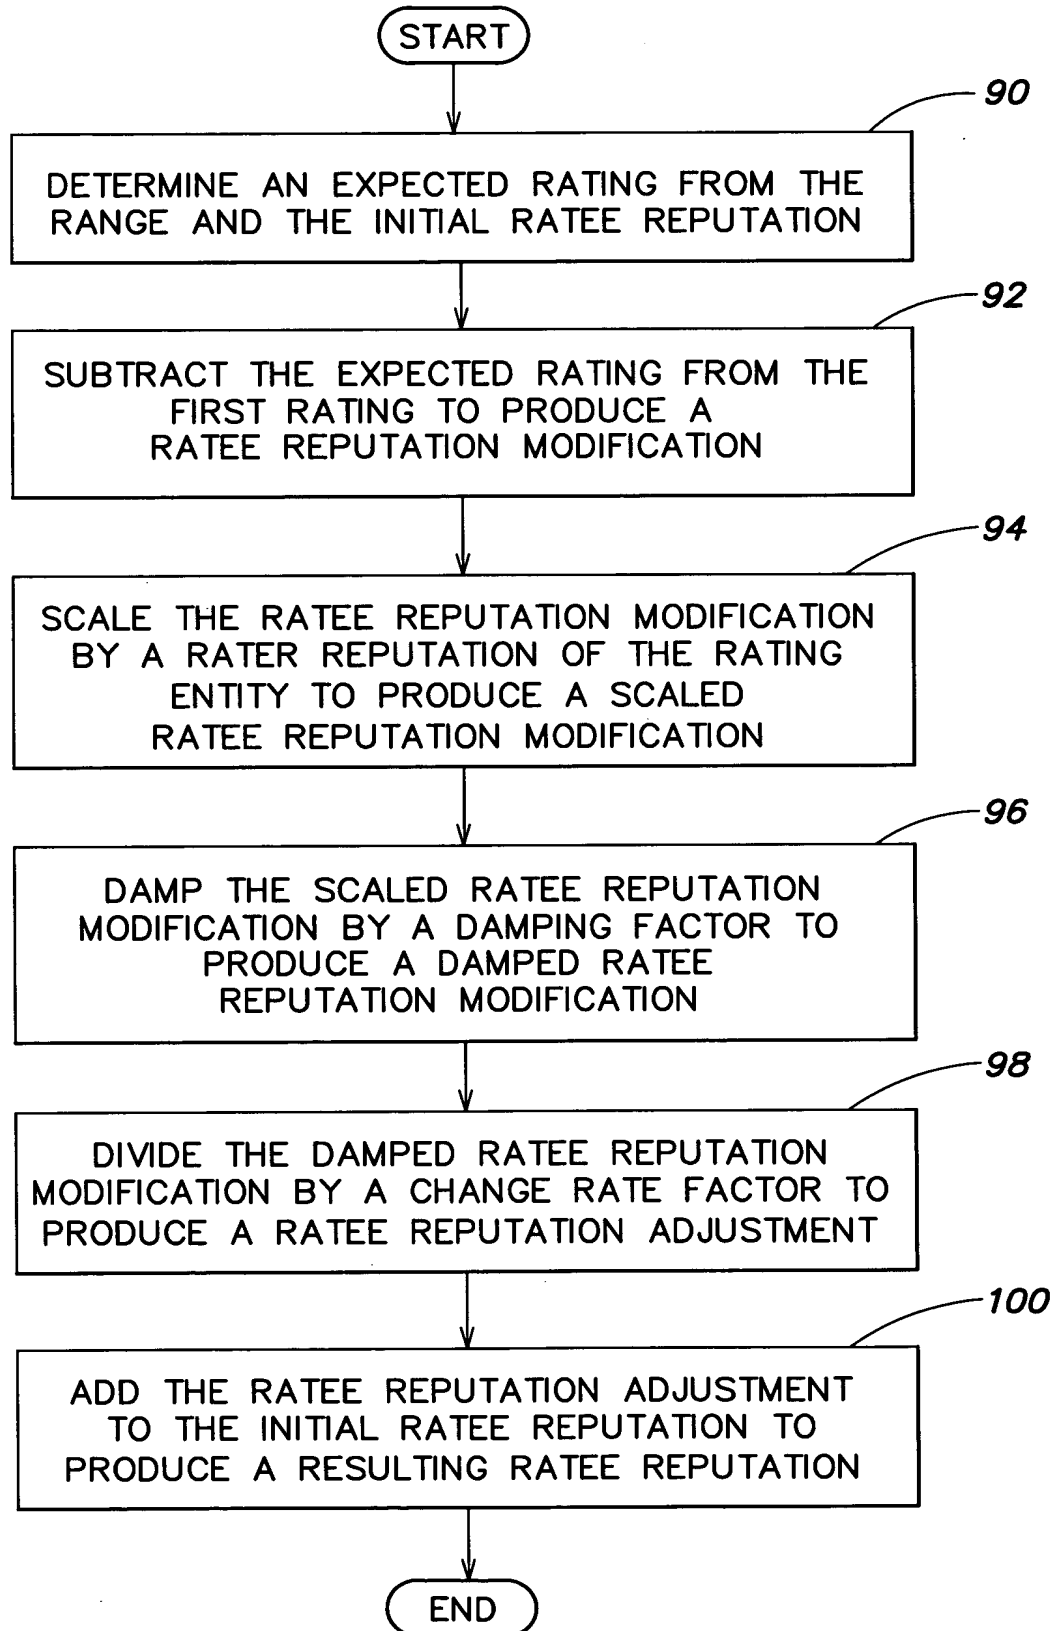

**FIG. 8**



10/19


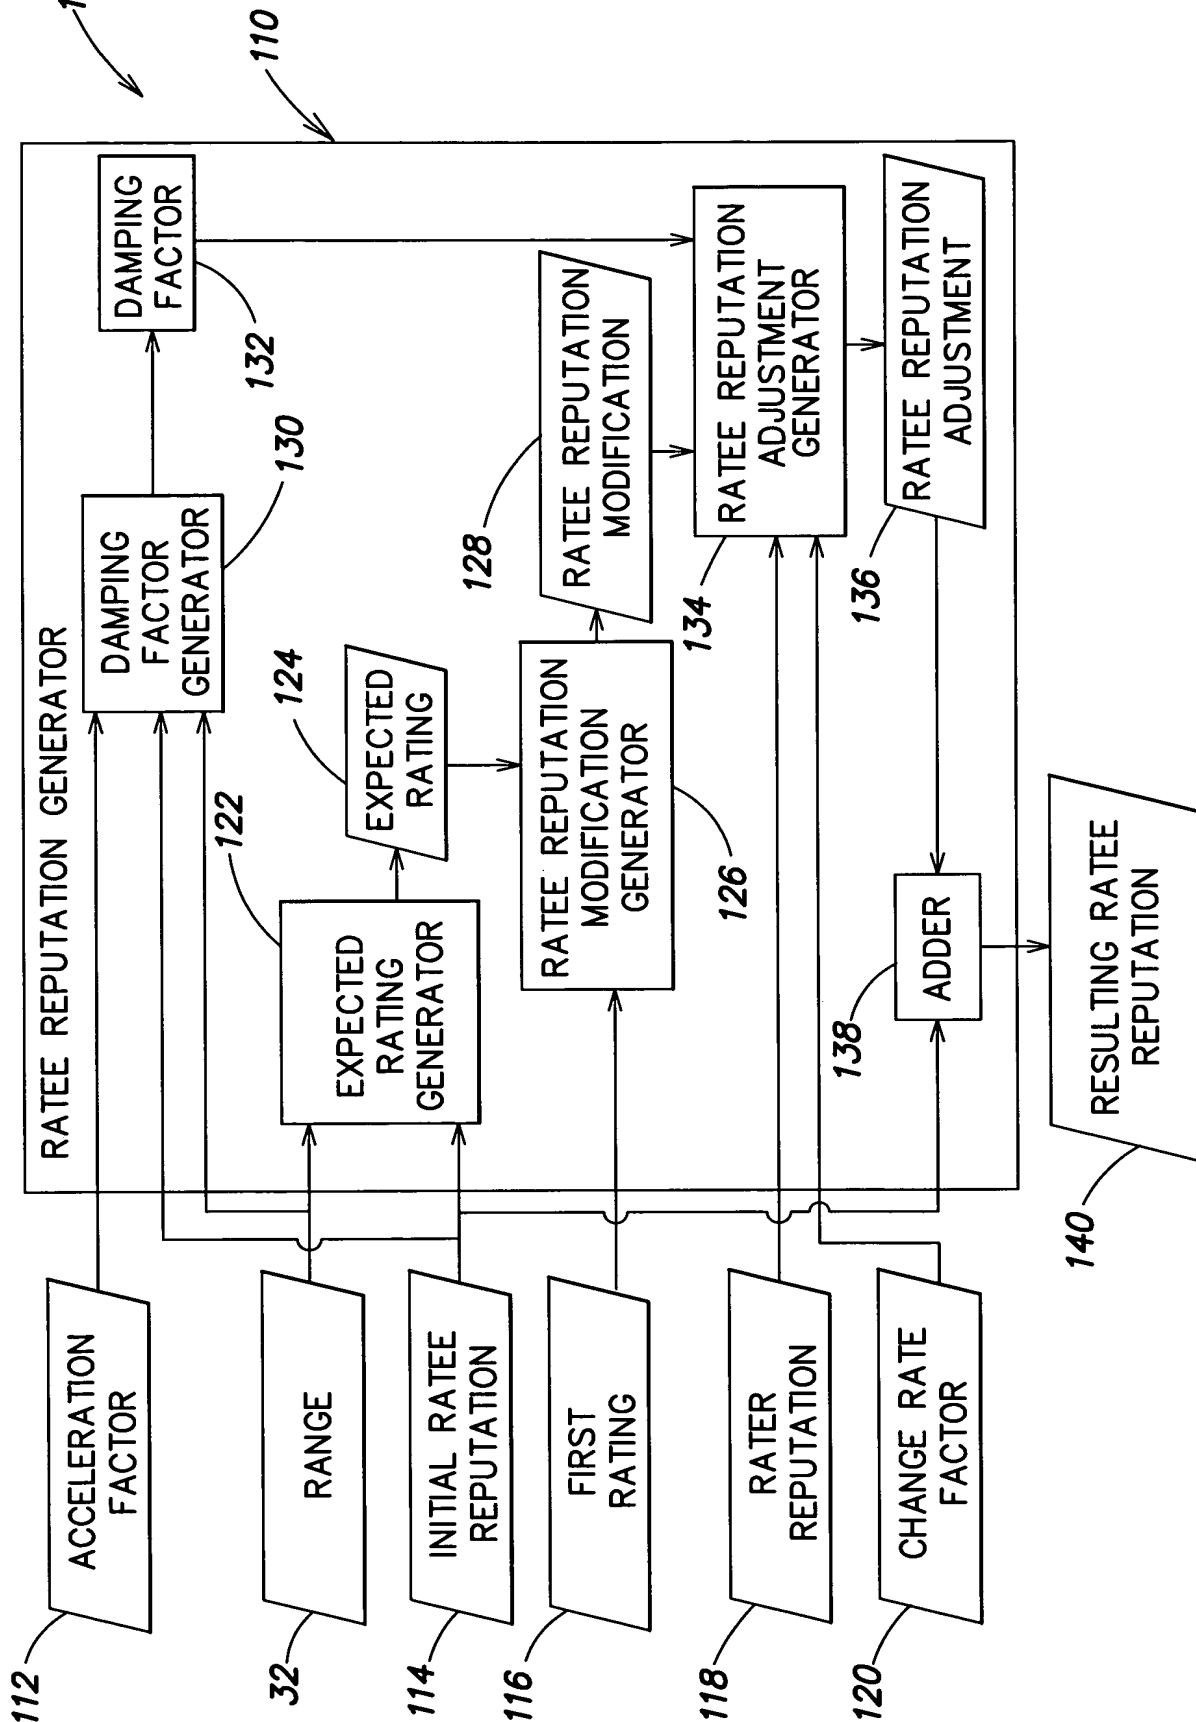


FIG. 9



11/19

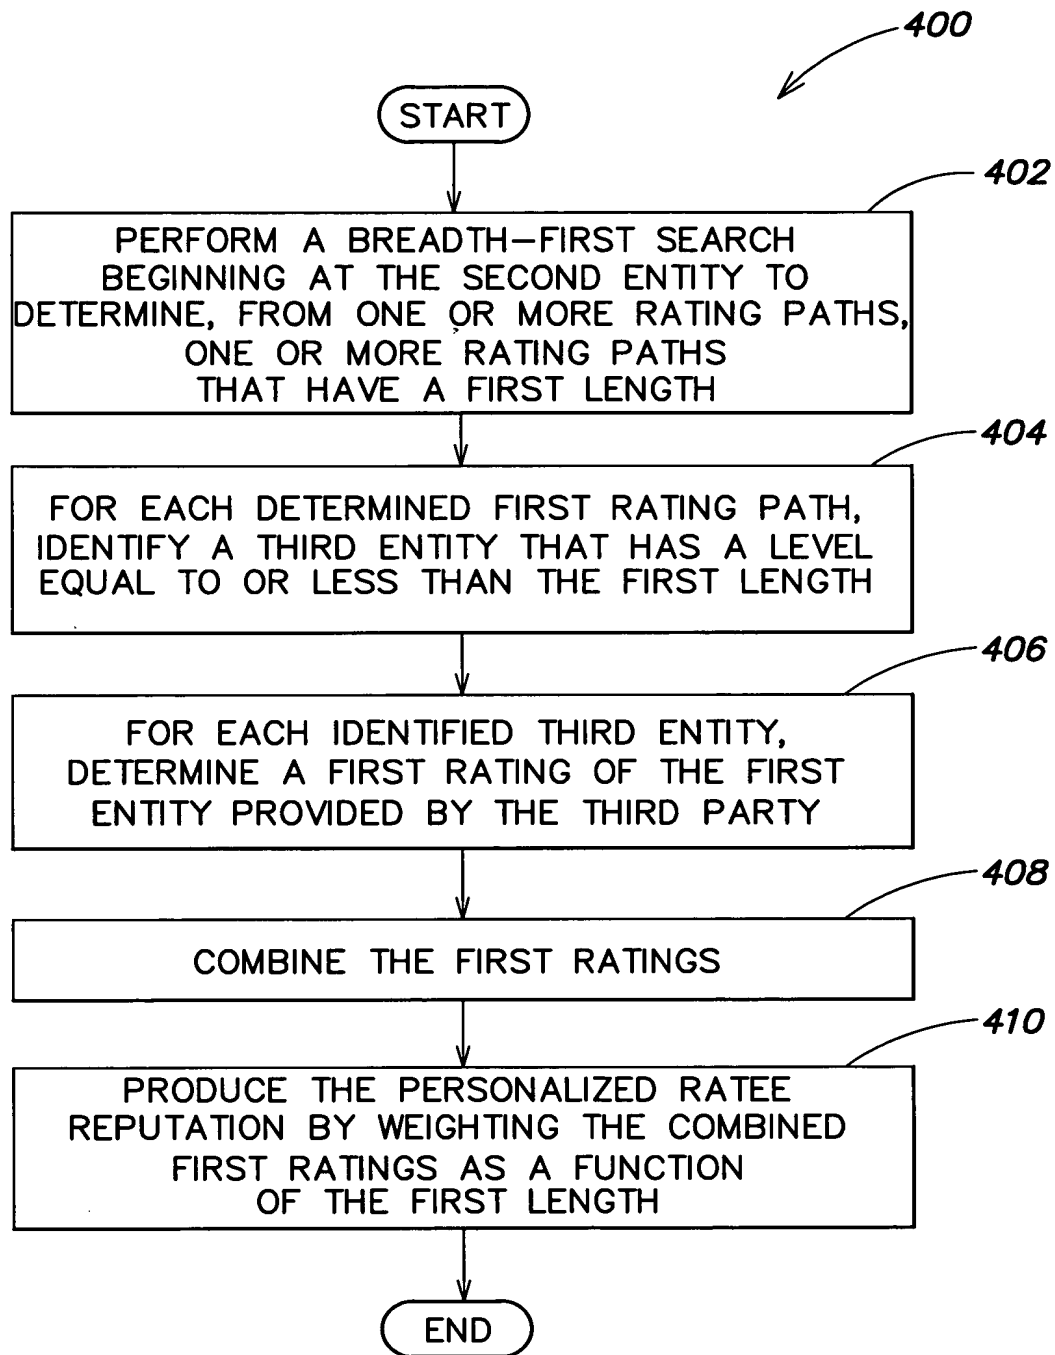

**FIG. 10**


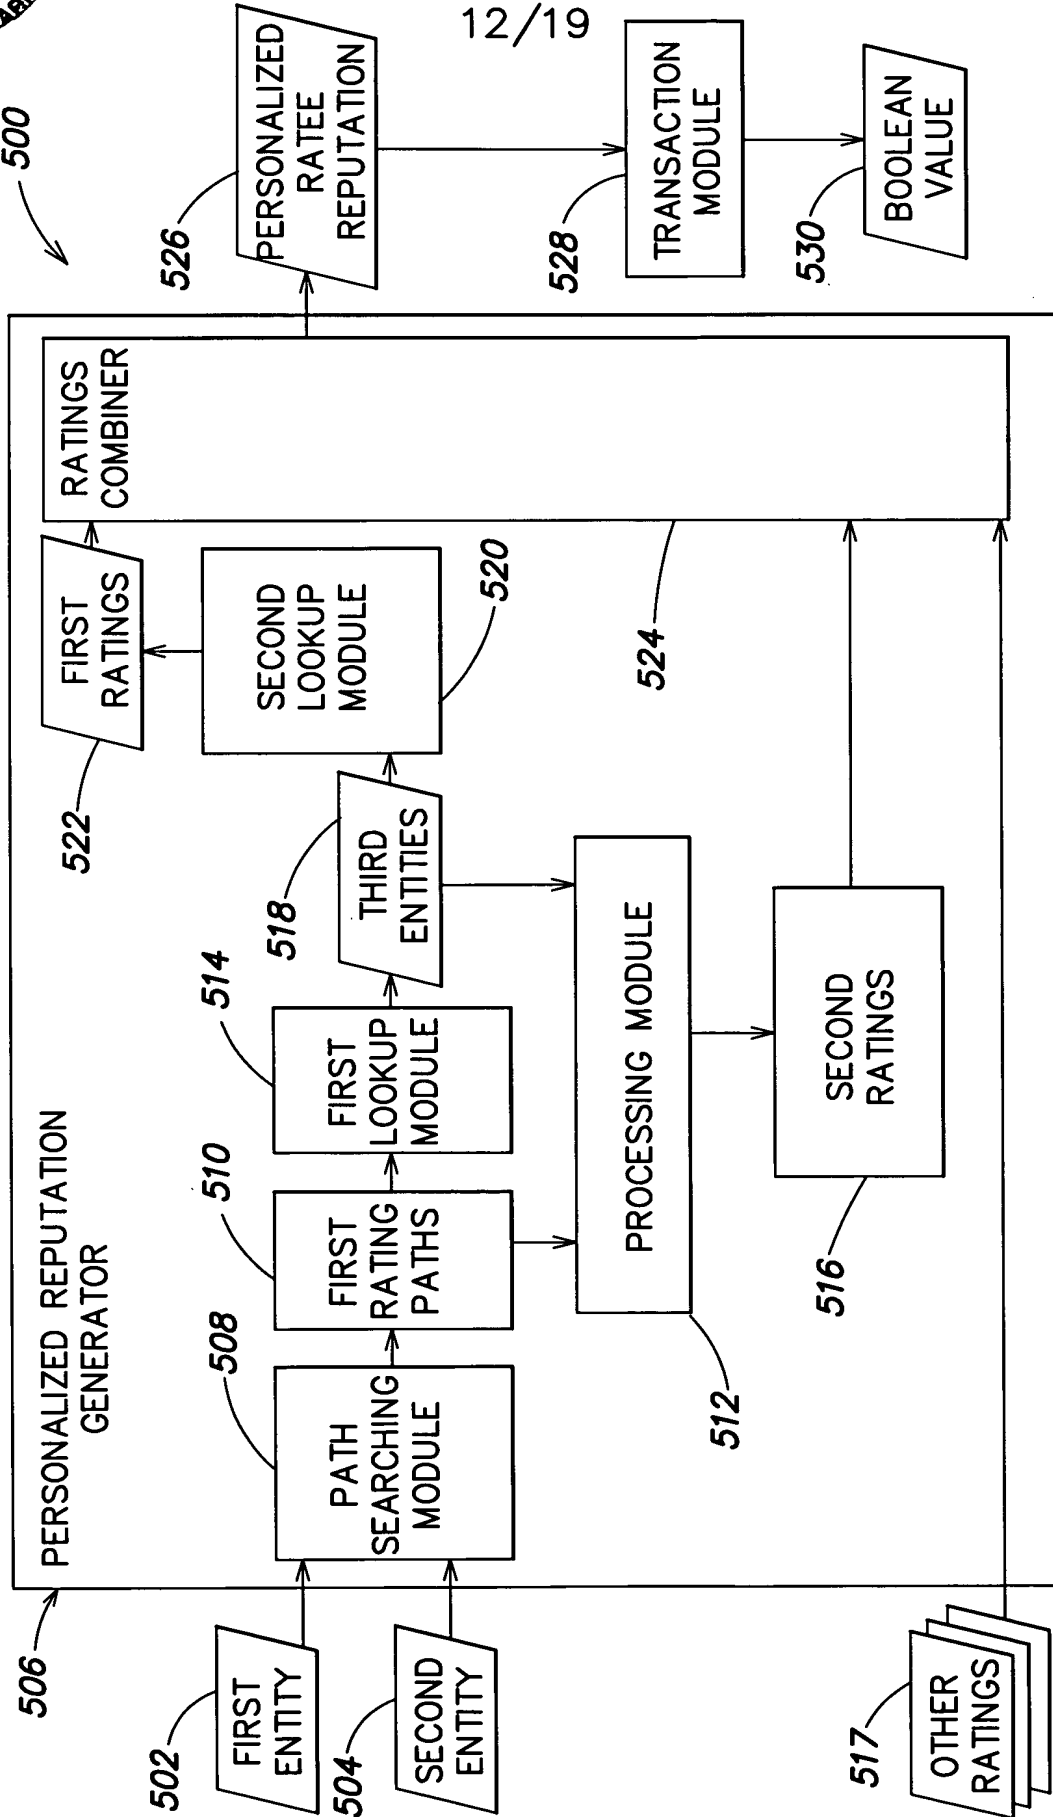


FIG. 11



13/19

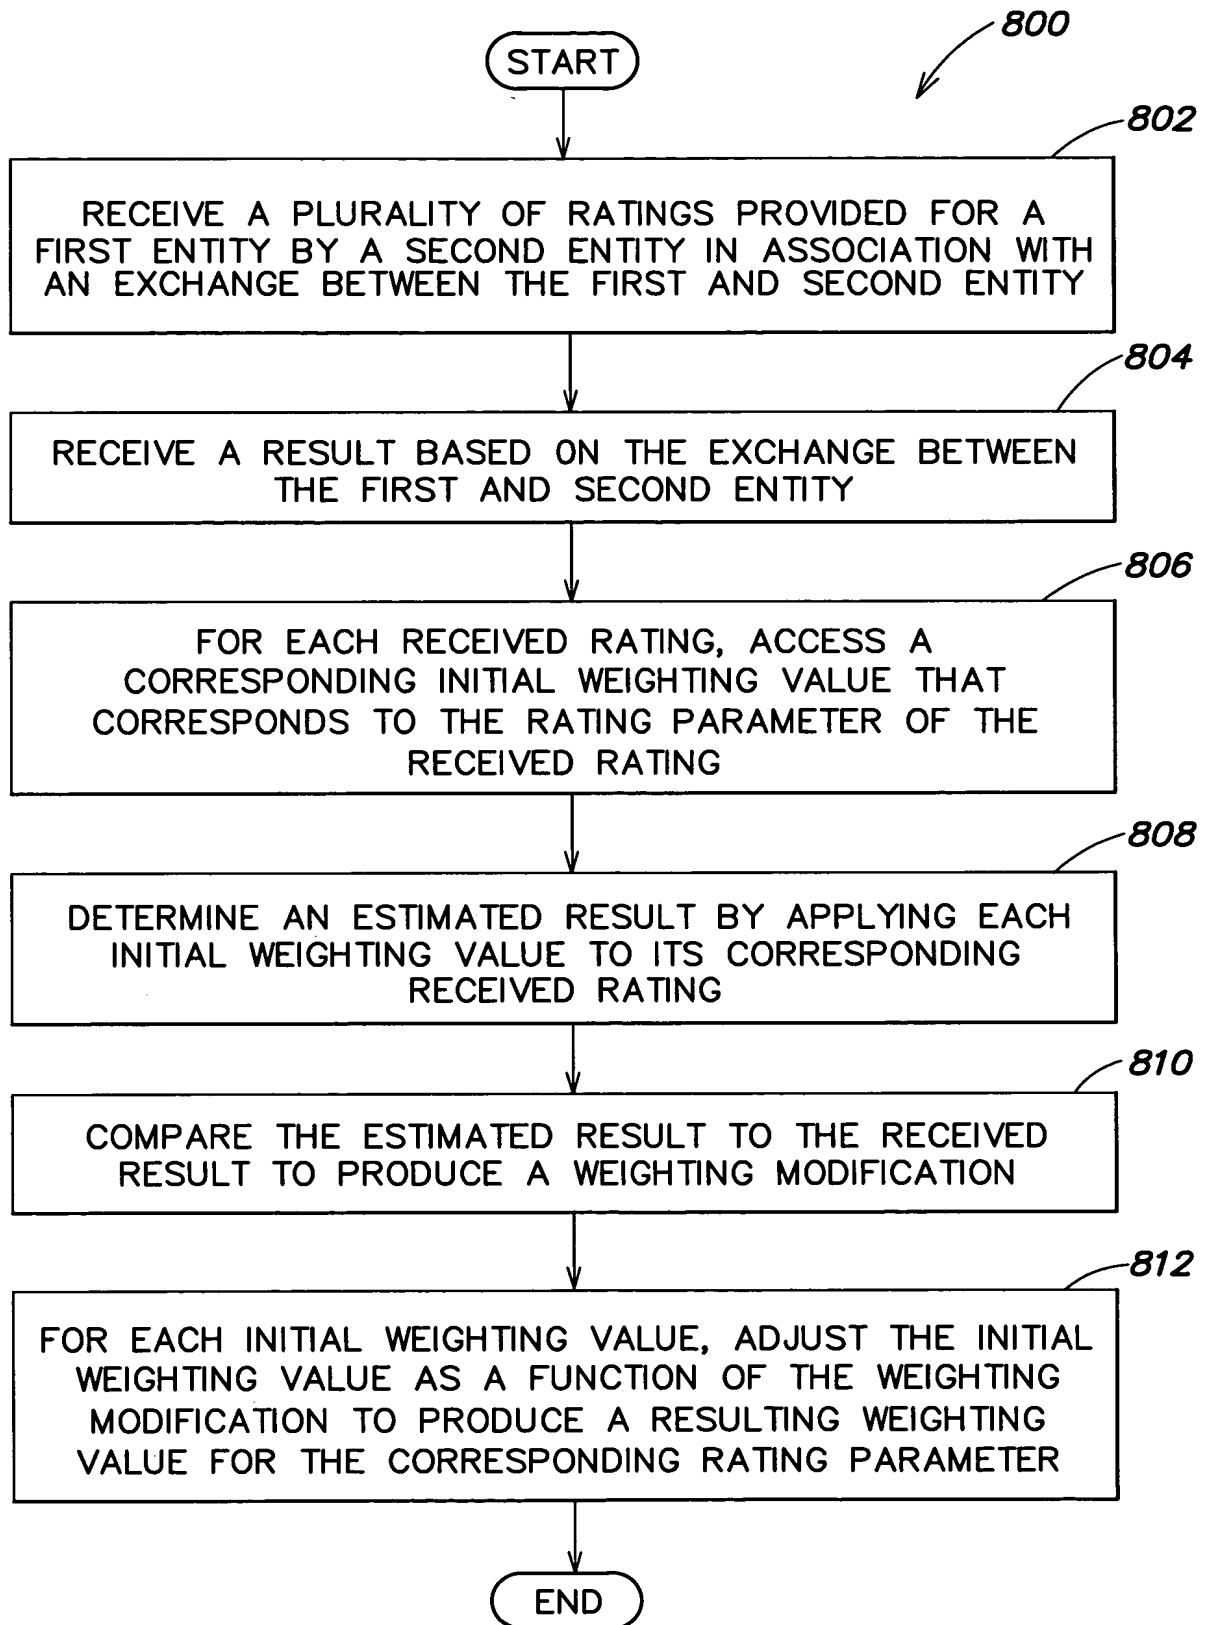


**FIG. 12**





15/19

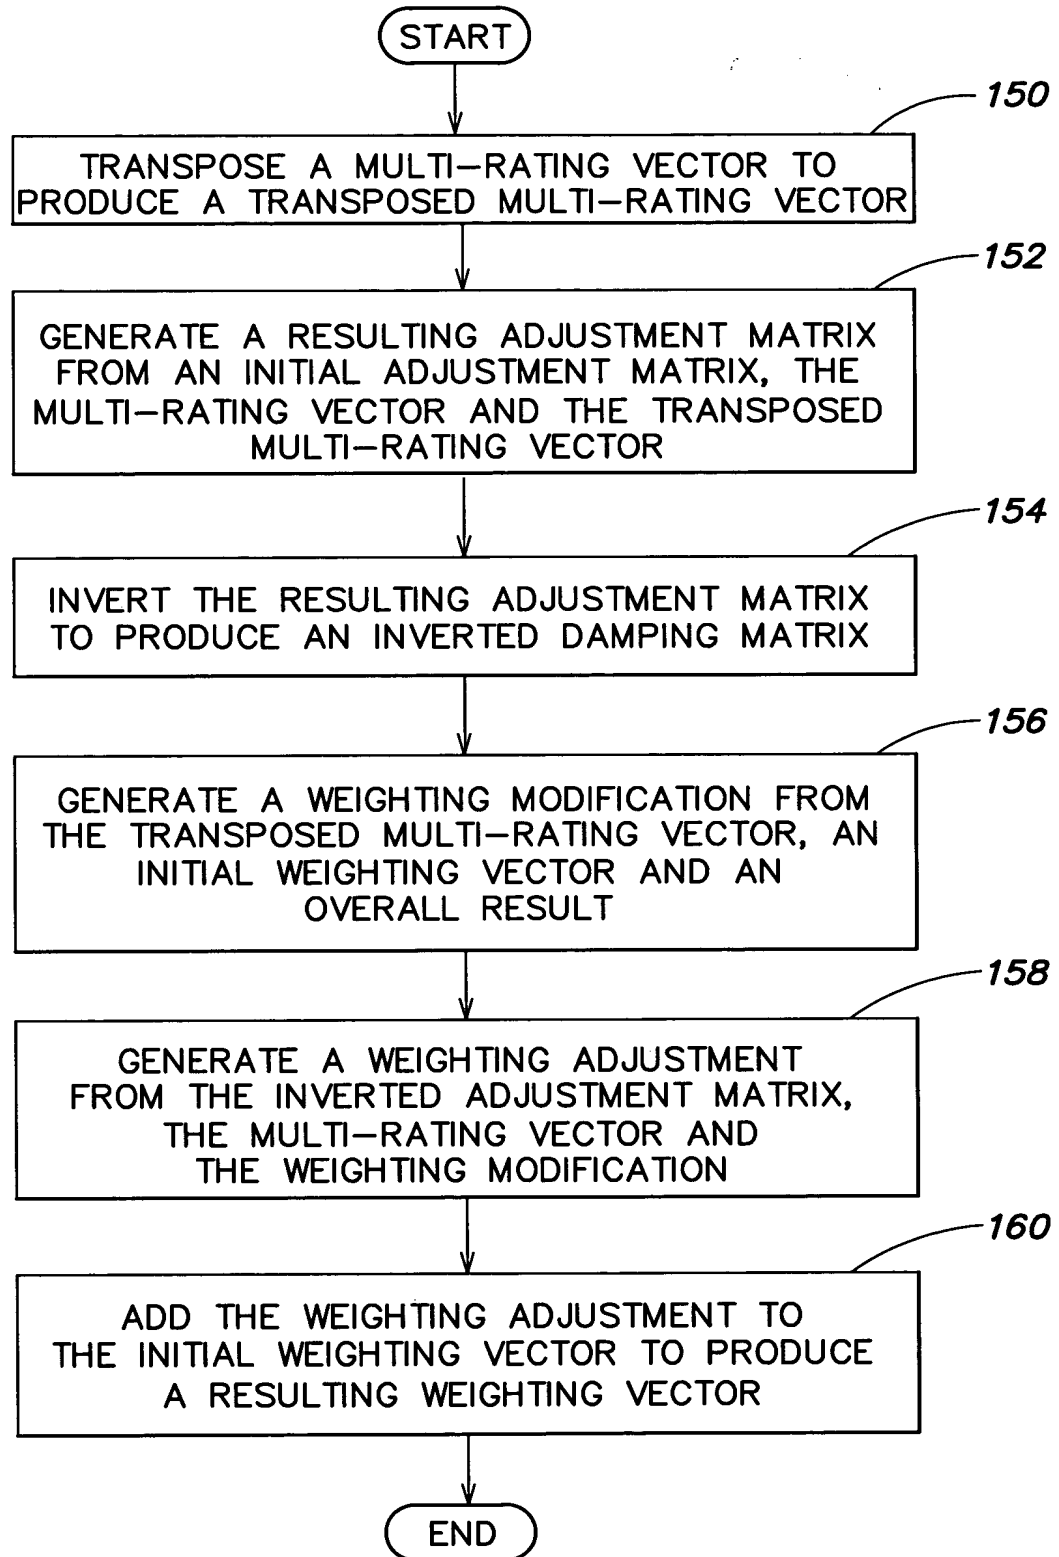

**FIG. 14**



16/19


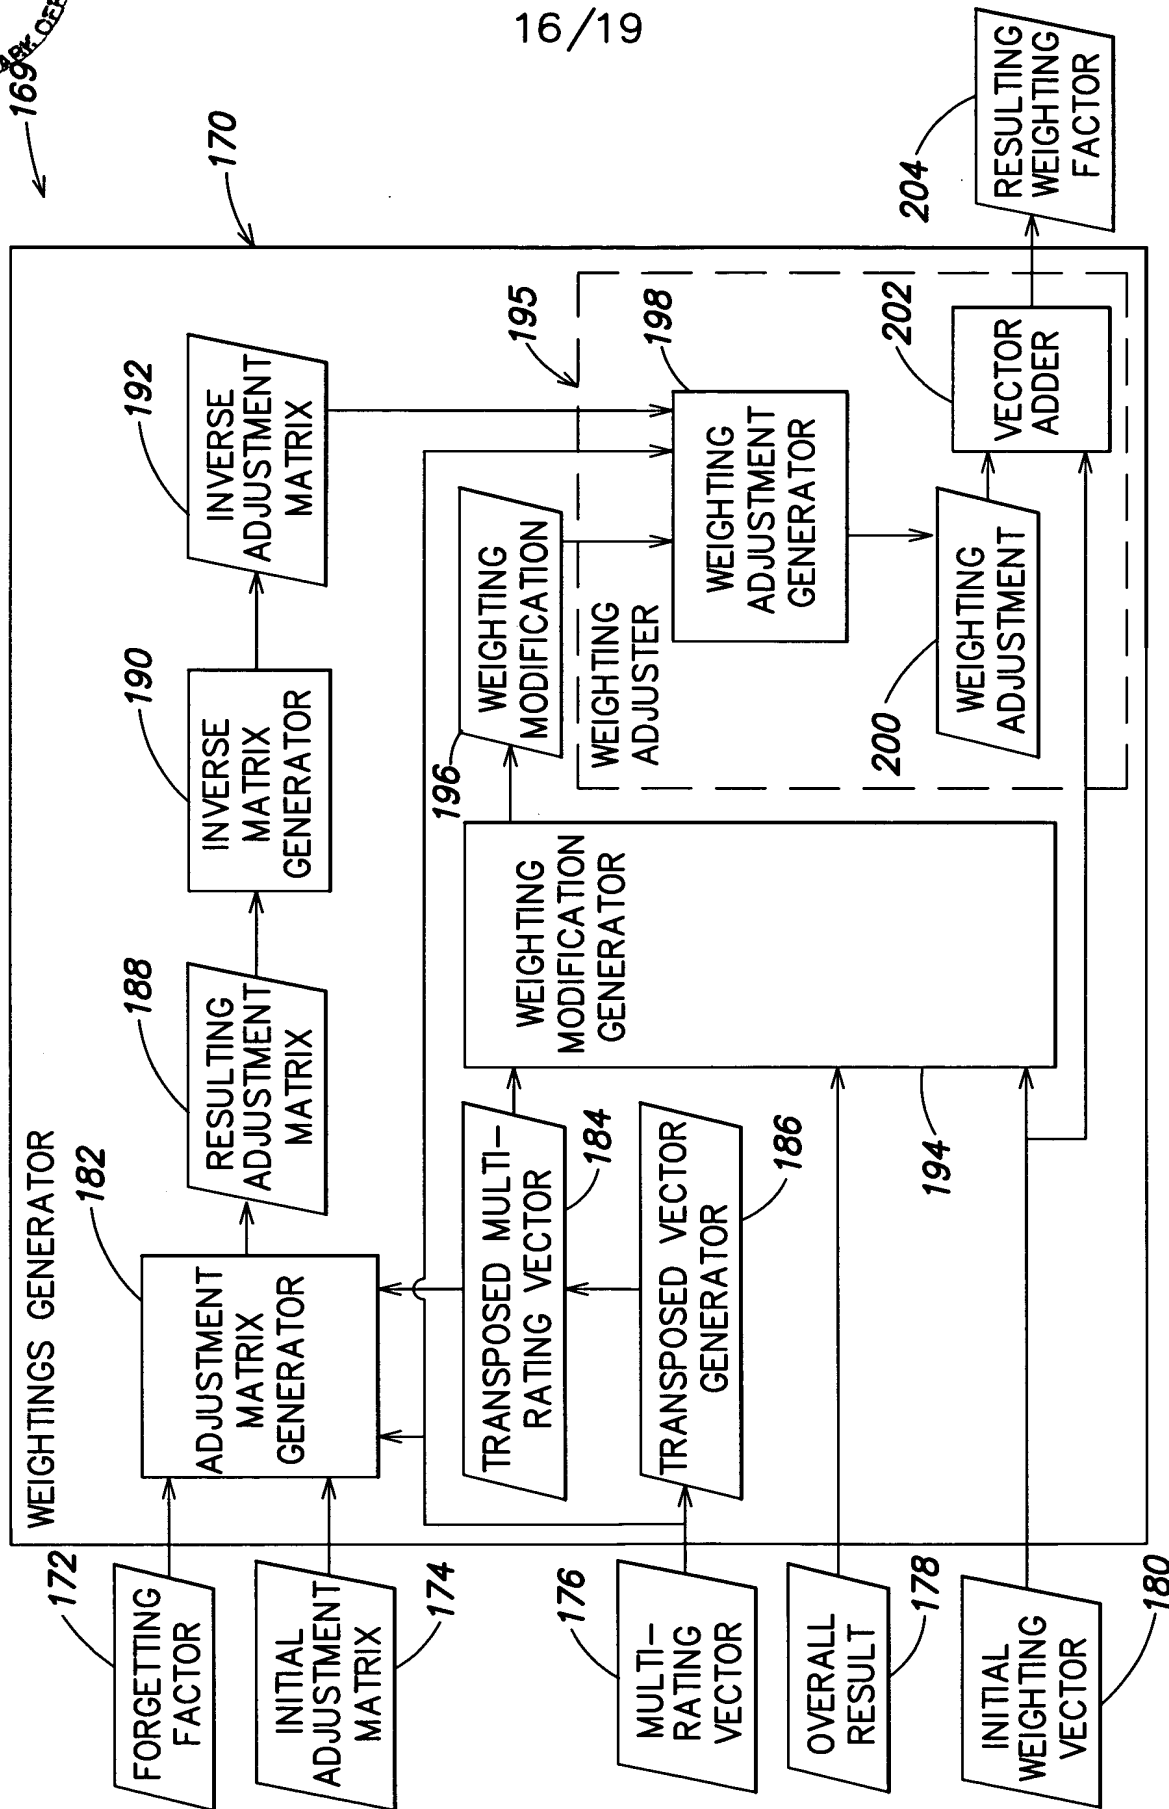


FIG. 15

17/19



**FIG. 16**

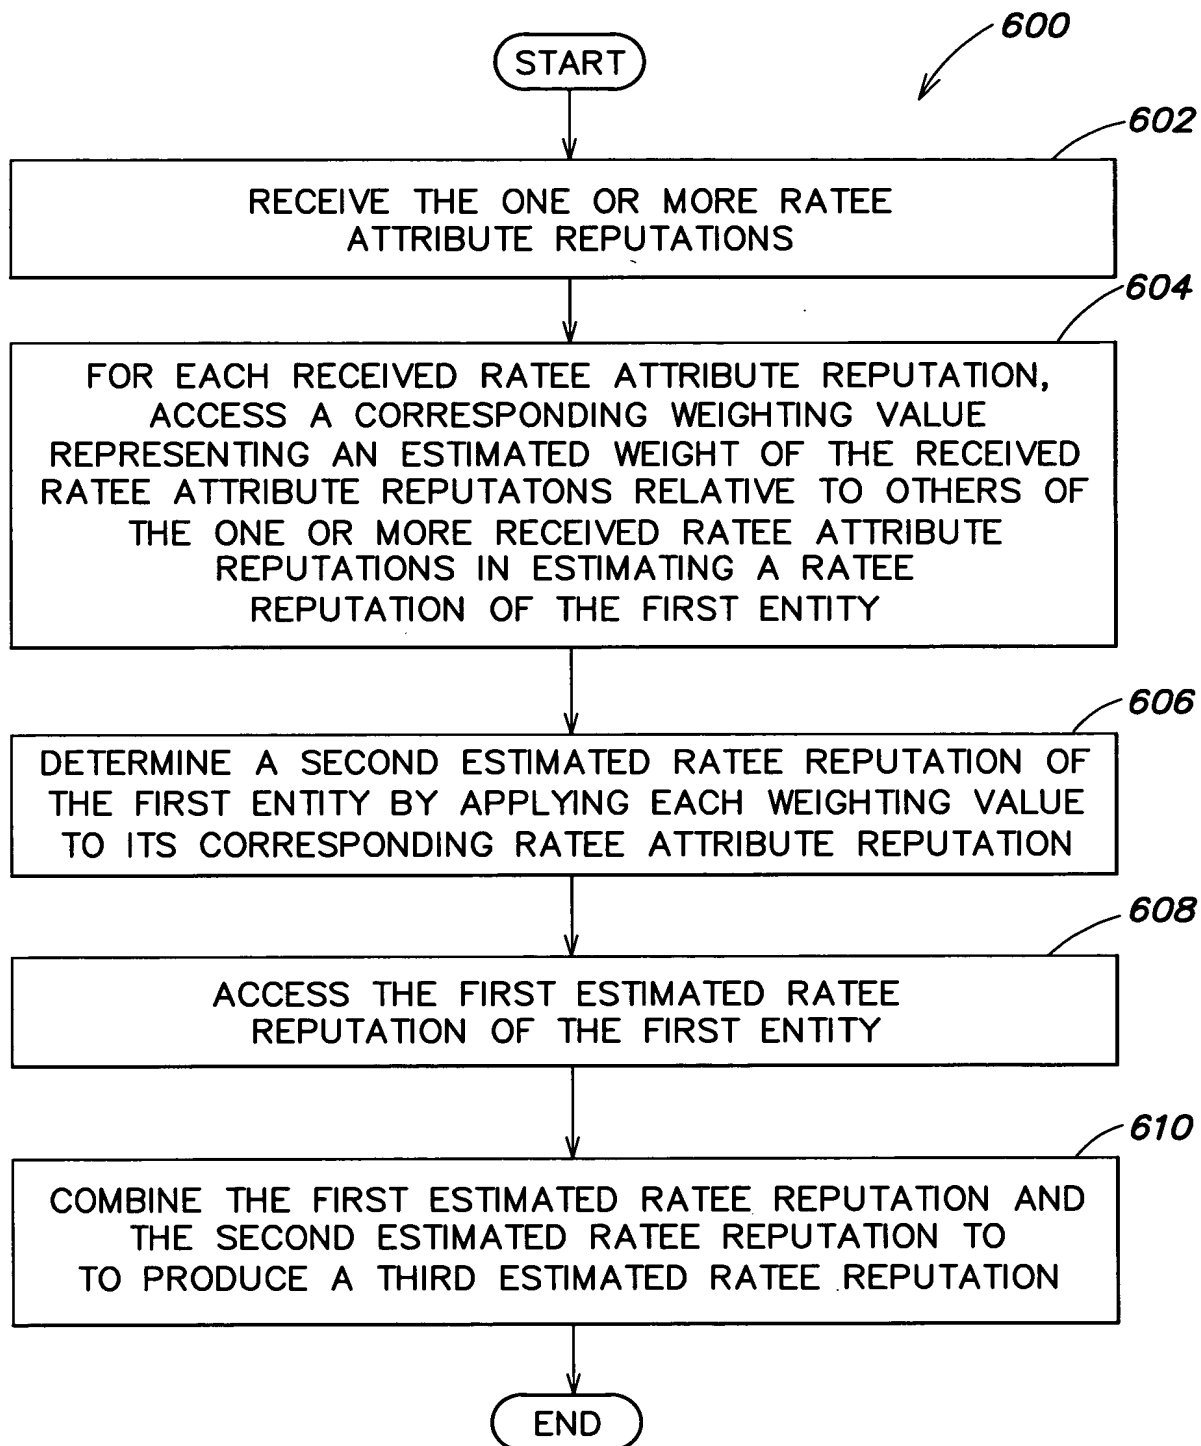

18/19

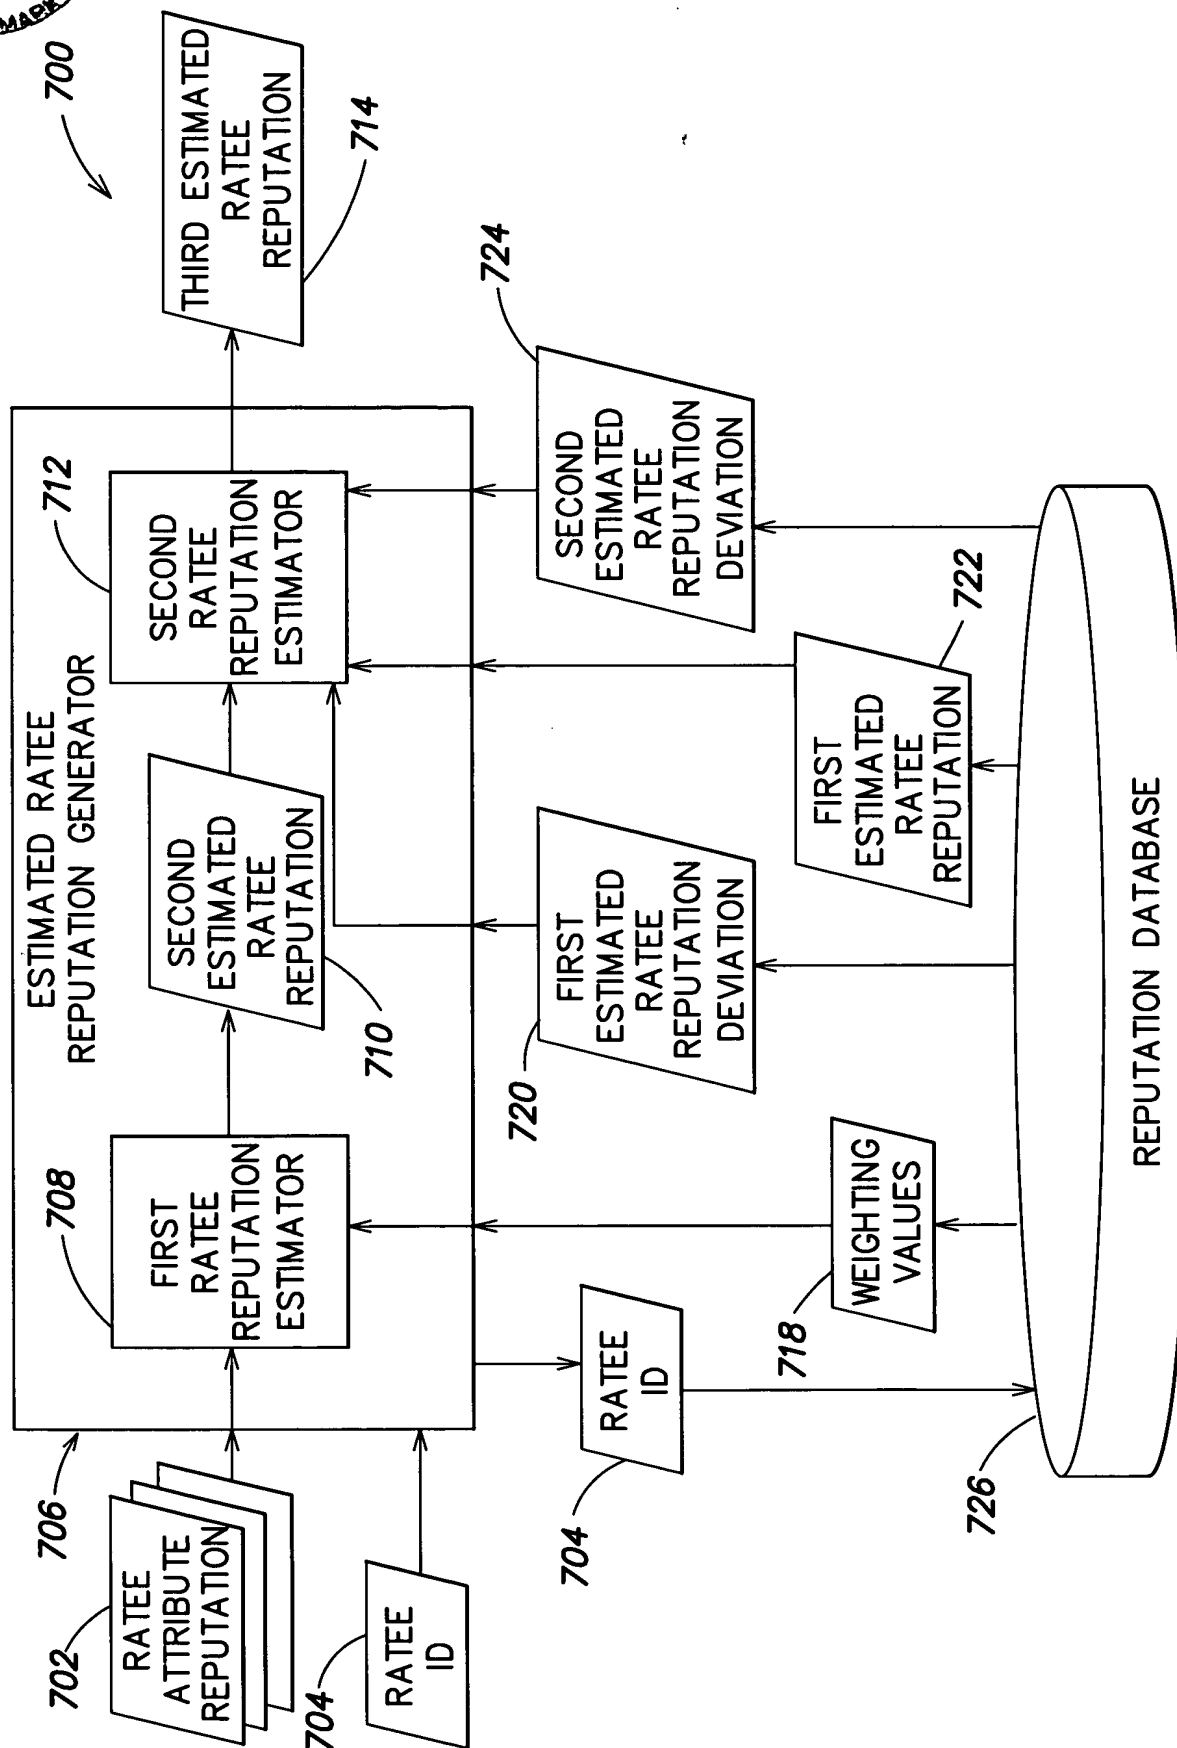


FIG. 17

